



**International Journal of Biology, Pharmacy
and Allied Sciences (IJBPAS)**

'A Bridge Between Laboratory and Reader'

www.ijbpas.com

REGULATORY AND TECHNICAL ASPECTS OF SAMD (SOFTWARE AS A MEDICAL DEVICE)

NAGALAKSHMI S^{1*}, SANGEETHA PRIYA S² AND ARAVIND R²

1: Associate Professor, Department of Pharmaceutics, Sri Ramachandra Faculty of Pharmacy,
Sri Ramachandra Institute of Higher Education & Research, (Deemed to be University),
Porur, Chennai – 600116

2: M. Pharmacy – Second Year, Pharmaceutical Regulatory Affairs, Department of
Pharmaceutics, Sri Ramachandra Faculty of Pharmacy, Sri Ramachandra Institute of Higher
Education & Research, (Deemed to be University), Porur, Chennai – 600116

#All authors equally contributed to this work

*Corresponding Author: Dr. Nagalakshmi S: E Mail: nagalakshmi.s@sriramachandra.edu.in

Received 4th Jan. 2023; Revised 25th March 2023; Accepted 6th June 2023; Available online 1st Feb. 2024

<https://doi.org/10.31032/IJBPAS/2024/13.2.7756>

ABSTRACT

Software is revolutionizing how doctors practice medicine, customers control their health, and patients and providers interact. Software that can perform advanced medical functions—software as a medical device—is a game-changing innovation in digital health technology (SaMD). SaMD may diagnose ailments, prescribe medications, and offer clinical treatment recommendations. The US FDA, EU, and Australia TGA also specified general platforms. To overcome the challenges while interpreting software product fits into the Medical Device framework, IMDRF has developed different guidance including Risk based categorization to determine possible levels of premarket reviews, and real-world evidence (RWE). IMDRF plays a similar function in enabling the regulators to risk-stratify submissions and focus resources on products that pose the greatest risk to patient safety. While SaMD products are not new, there are many new players in the SaMD space to better regulate iterative devices. One of the key goals is to identify the excellence of the SaMD Regulatory paradigm regulation of these products will need to radically change to accommodate new SaMD manufacturers and the technology's rapid evolution and to harness SaMD's ability to capture RWD to create a

collaborative, innovative SaMD community. This review aimed to describe the Regulatory and Technical aspects of the software as a medical device and regulatory transformation of digital health rapidly expanding regulations by different Health Authorities.

Keywords: SaMD, IMDRF, Risk Categorization, ISO/IEC, Application Lifecycle Management, GDPR

INTRODUCTION

Prospects for (SaMD) products are quite promising. This program has the potential to not only enhance the identification and treatment of ailments but also grant people a greater degree of autonomy when it comes to their health. Moreover, the data collected by these goods can expedite the process of innovation and lead to more advanced algorithms. SaMD refers to a software program that functions as an independent medical product and should not be confused with SiMD, which is simply software that helps medical device hardware to operate. The most significant characteristic of SaMD is that it can carry out medical tasks without needing hardware. It is usually used in conjunction with non-medical computer systems linked to the internet, regular medical devices, or other basic computing platforms.

Medical device definition

A medical device is any type of equipment, tool, implant, reagent, software, material, or

other article intended by its maker to be used in humans, either independently or with other items, for one or more particular medical purposes [1].


In vitro diagnostic (IVD)

In Vitro Diagnostic (IVD) medical device' means a medical device, whether used alone or in combination, intended by the manufacturer for the in-vitro examination of specimens derived from the human body solely or principally to provide information for diagnostic, monitoring, or compatibility purposes [1].

SaMD definition

The International Medical Device Regulatory Forum (IMDRF) defines SaMD as "software designed to be used for one or more medical purposes to perform those operations that are not part of the medical device. It serves individual patient-specific medical purposes (i.e. a specific disease or condition) [1].

Medical software use falls into four categories [2]

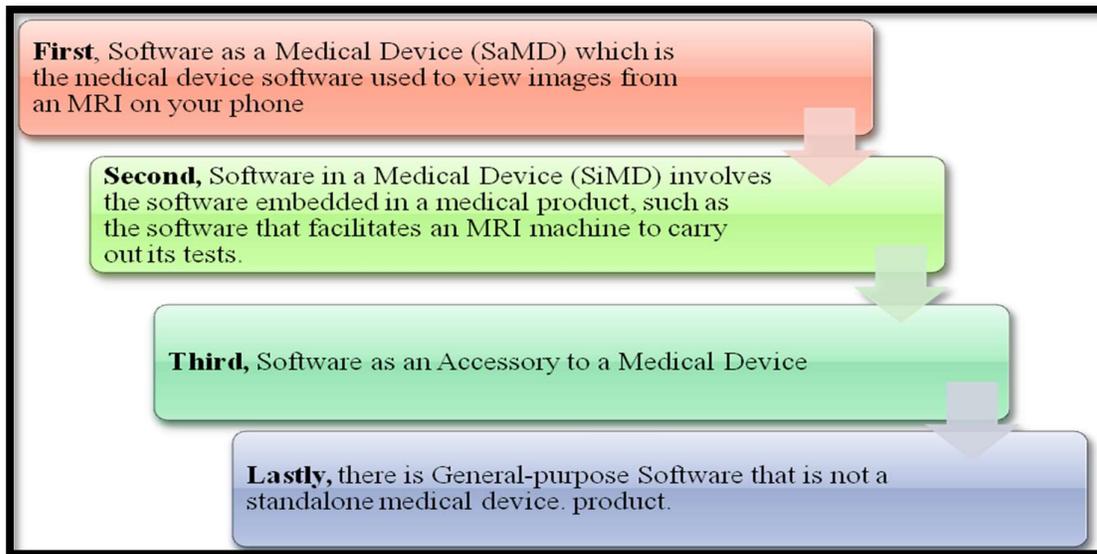

Some of the primary features of SaMD are

Data-driven better health outcomes:

SaMD has the potential to augment existing medical treatment methods and equipment.


Speedy production and feedback for accelerating innovation:

SaMD can supplement the existing medical devices and bring about faster software solutions that are more affordable to upgrade than hardware.

This facilitates rapid manufacturing and feedback, thus speeding up the process of innovation [2] [14].

SaMD basic programming model

The SaMD programming model is a form of software that takes digital content as the input and, based on a set of rules and a model, produces an output that is designed for use in the Medical Field [2].

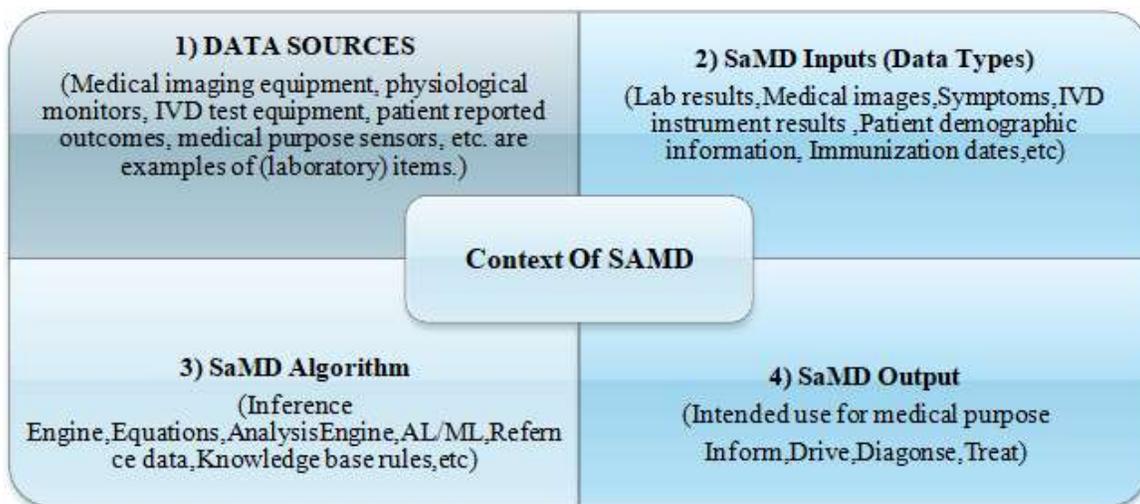

What is and is not SaMD? [2]

SaMD	Not SaMD
The program can calculate the right dosage of medication for a patient based on their unique patient data.	Software that is used to operate a pacemaker. CRM (customer relationship management) software.
Program analyzing MRI images that can recognize and classify strokes	The motor-driving or -controlling software for an infusion pump.
Software that can track the development of a mole over time and assess its likelihood of developing melanoma.	Systematic use of electronic health records. the patient portal computer-aided coding Automated tools for patient scheduling.
Software that analyses information from various using technology techniques to assess the risk variables linked to epileptic seizures	Equipment that assembles medical devices.

A rational perspective on risk categorization of software as a medical device

The severity of the medical device and the output of the software—provide information for clinical management, treatment monitoring, and therapies used to determine the IMDRF SaMD risk level. To assist businesses in assessing the risk associated with using the software as a medical device, the IMDRF Framework was created (SaMD) [3].

SaMD Categorization Principles

To effectively categorize SaMD, certain fundamentals must be in place. Specifically,

the categorization is dependent on having a precise and thorough SaMD definition statement. Moreover, the categorization is achieved by considering the importance of the data obtained from SaMD in making healthcare decisions and managing a specific medical condition or scenario. The following categories are based on the scope of the SaMD's influence on patients or public health (I, II, III, as well as IV). For the public's health to be protected and to prevent death, permanent disability, or any other major deterioration in health, the SaMD's information must be accurate [3].

CATEGORY I	CATEGORY II	CATEGORY III	CATEGORY IV
Astigmatism may be diagnosed using software that analyses pictures and eye movement.	Software that monitors heart rate	The software detects irregular breathing using a microphone	Software that can perform diagnostic image analysis
Computer programs that record blood pressure data for later.	Health data analysis software can be used to forecast the risk of cardiac ailments and estimate the likelihood of asthma attacks.	A lesion's fractal dimension is computed via software.	Software that produces a structural map with potential development patterns
Software to help with hearing loss self-evaluation	Software that integrates tests and analyses the results to suggest a diagnosis	-----	Data-combining software that searches for changeable pathogens by combining information from several sources

SaMD in Action

1. Screening and diagnosis:

Computer programs that use advanced algorithms can accurately predict the possibility of acquiring a chronic ailment and aid in determining the optimal course of therapy.

2. Observation and notification:

Several vital indicators may be captured using wearable sensors in SaMD systems, and these data can subsequently be followed using the software. The computer records this information and utilizes it to provide precise suggestions and warnings to patients and clinicians.

3. Management of recurrent illnesses and diseases: SaMD is a tool that

both patients and doctors may use to collect and understand health data and modify treatment plans for better outcomes.

4. Computerized therapies: SaMD is

helpful for both treating and preventing serious illnesses its capacity to collect and input highly pertinent clinical data into "other medical devices, pharmaceutical product special-purpose transducers, or other ways of administering treatments to a human body [2] [4].

International regulations and technical aspects [2] [4]

In 2013, the International Medical Device Regulators Forum established a committee centered on software as a medical device (IMDRF). They are investigating the

characteristics that distinguish this type of software. The related documents can be accessed on the IMDRF Journal articles website in the "Technical documents" area [1] [2] [3] [4].

The Worldwide Electrotechnical Commission (IEC) is an international organization that creates and circulates global standards for all types of electrical, electronic, and related technologies (commonly referred to as "electro technology").

ISO, an independent, non-governmental organization, offers a unified framework to

ensure the overall performance, safety, and quality of goods and Systems.

The IEC 62304 is a regulation in the medical area that is especially pertinent to the production and upkeep of medical device software. To guarantee that regulations such as the FDA 21 CFR Part 820 and ISO 13485:2016 are followed, SaMD suppliers must incorporate a strong quality control system into the building process. The FDA, Health Canada, and the MHRA have created standards for the development of GMLP [5] [6] [7].

Major used standards (standard for compliance) [5] [6] [7]

Apart from the FDA's and IEC 62304 regulations, there are also other regulatory standards for medical devices

- [ISO 13485](#) — quality management
- [ISO 14971](#) — risk management
- [EU Medical Device Regulation](#) — EU standard which replaces Medical Devices Directive in 2020
- [IEC 62304 - Medical device software - Software life cycle processes](#)


Standards related to software as a Medical device are to be followed

- IEC 82304: Safety and reliability of healthcare software products
- IEC 62366: Usability requirements for medical devices
- ISO/TR 20416: Post-marketing monitoring (under the manufacturers' responsibility)

Implementing the IEC 62304 standard's requirements into the software lifecycle

A Software Quality Assurance Plan must include the IEC 62304 to achieve its software lifecycle criteria, and Application Lifecycle Management is crucial for the development of embedded software

products. Therefore, using an efficient ALM solution is essential for developing and monitoring software quality in the medical industry. It enables effective monitoring of the full application lifetime and supports both on-site and remote audits [5] [6].

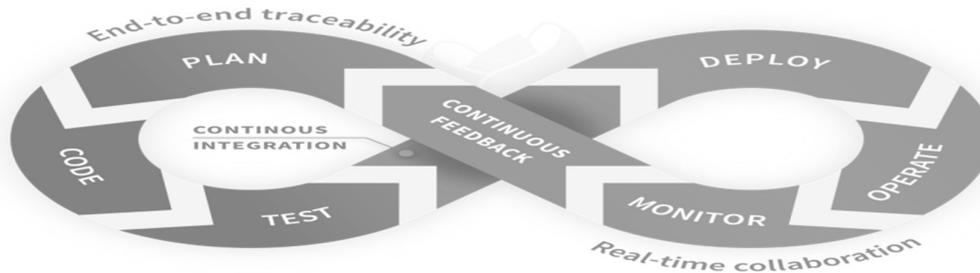

IMPLICATION OF SECURITY CLASSIFICATION FOR SOFTWARE ENGINEERING

MEDICAL DEVICE CLASSIFICATIONS				
Regulatory Agency	LOWEST \rightleftarrows HIGHEST			
International (IMDRF)	I	II	III	IV
EU(MDR)	I	IIa	IIb	III
EU(IVDR)	A	B	C	D
USA(FDA)	I	II	II	III
SAFETY/RISK CLASSIFICATIONS				
Regulatory Agency	LOWEST \rightleftarrows HIGHEST			
International (IEC 62304)	A	B	C	
USA(FDA)	Minor	Moderate	Major	

Software Verification and Validation Plan That Includes [7]

Software Verification And Validation Plan That Includes

- **Design management:** The ability to store and monitor all of the numerous versions and modifications that a system will employ makes configuration management an essential part of the software lifetime (physical components, programming, records, output data, etc)
- **Change Control**
- **Defined development process**
- **Requirements traceability management:** Many firms still use labor-intensive, complicated, and—more importantly—prone to mistake, manual tracing approaches. Utilizing tools that provide automatic traceability between project components while simultaneously reducing risks is crucial.
- **Defect detection and software vulnerability identification**
- **Risk management and Risk Mitigating Management**

Clinical Evaluation

The US FDA, EU, and Australia TGA have also said that generic platforms on which such medical software may operate or be

distributed are not intended by their maker to be used for therapeutic purposes and would not be regulated as a medical device [8].

STAGES	CLINICAL EVALUATION	REMARKS
STAGE - 1	VALID CLINICAL ASSOCIATION	Exists a reliable clinical correlation between your SaMD's output and the clinical problem it was designed to treat?
STAGE - 2	ANALYTICAL TECHNICAL PERFORMANCE	Does your SaMD properly analyze input data to provide exact, accurate, and trustworthy output data?
STAGE - 3	CLINICAL PERFORMANCE	Does the utilization of your SaMD's accurate, dependable, and exact output data enable you to accomplish your goals about your target audience when providing clinical care?


Regulatory framework [8] [9]

FDA's approach to regulation for software-based medical devices

QSR Requirements for Medical Devices, Part 820, Drug Quality System Regulation. According to the FDA's Digital Health Innovation Action Plan, protracted approval processes for SaMD product upgrades may keep patients from receiving life-saving devices. Whether inventors file a 510(k) application (Traditional, Special, and Abbreviated submissions), a self-registration form or a Premarket Approval

(PMA) application will determine how long the FDA will take to approve a medical device. Application De Novo **Principles and solutions for a new regulatory framework** Patients who stand to gain from new digital health technologies, SaMD product developers, and regulatory agencies are all involved. The FDA has developed a five-part action plan to help it regulate SaMD-based devices better in 2023 and beyond [8] [9] [12] [14].


(Total Product Lifecycle Management)
The plan involves the following steps [9]

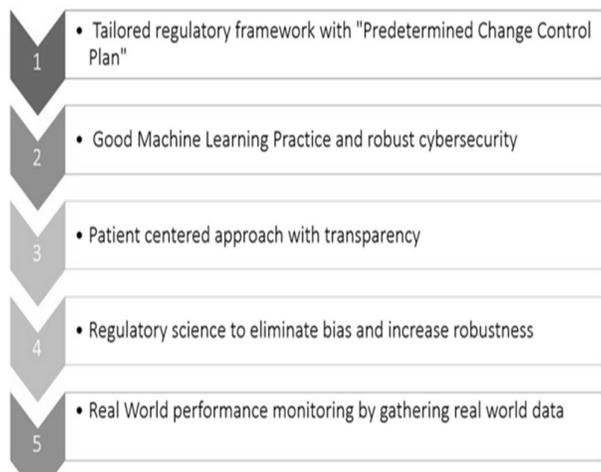

The following concepts constitute the TPLC scheme

The FDA TPLC approach would make it possible to assess businesses and their SaMD products over the course of their

lifecycles (from premarket development to post-market performance), giving patients, carers, and other users confidence in the products [8] [9].

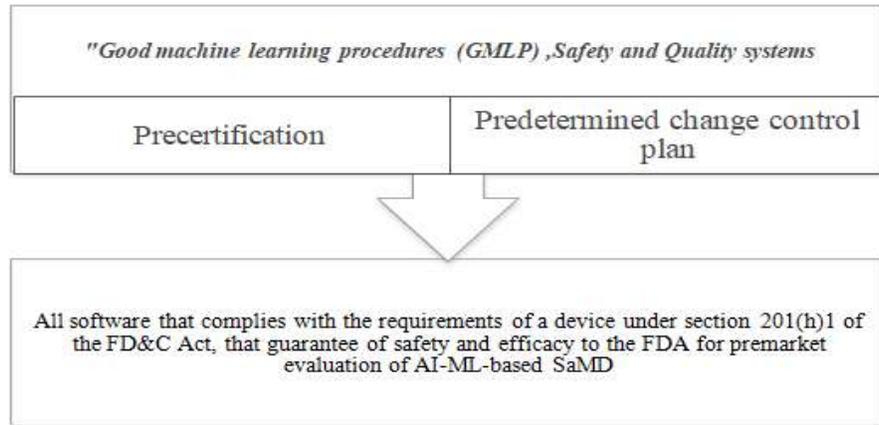

The plan anticipates two types of modifications:

- SaMD specifications (SPS) - When the SaMD is already in use, model adjustments and reorientations are necessary.
- The Algorithm Change Protocol (ACP) manages the risks to patients by implementing the modifications in a controlled way

The Software Pre-Cert Program model will be tested by the FDA before it is used as an alternative premarket pathway for SaMD.

There are 4 key application components [12]

- **Excellence Appraisal**
- **Review Determination**
- **Streamlined Review**
- **Real-world**

“RWE (*real-world evidence*) in USA medical device regulations” [8] [9]

Incorporating RWE into regulatory decision-making is strongly encouraged by the FDA.


In post-marketing approval and surveillance, examples of RWE and RWD include

- RWE in post-marketing approval for expansions of • Bayesian hierarchical analysis was utilized by the sponsor in post-marketing clearance for the extension of indications. RWD was taken from two registry datasets.
- RWD in post-marketing surveillance –Post approval research was carried out to assess efficacy and safety [14].

EU (Mdr) Medical Device Regulation for Software-Based Medical Devices: Regulatory Approach

The EU Medical Device Regulation (MDR; 2017/745) and the EU in Vitro Diagnostic Regulation (IVDR; 2017/746) apply to medical devices and in vitro diagnostic devices, respectively. Europe's Commission and the Medical Device Coordination Group are developing SaMD legislation (MDCG). The MDCG is a professional group that has been chosen to monitor a wide range of topics, including notified bodies, clinical research, post-marketing surveillance, international concerns, the deployment of the EUDAMED database, and recommendations for the use of IVD and Annex IV products. [11] [12] [14]


Medical Device Software(MDSW)can be placed on the market in two different ways

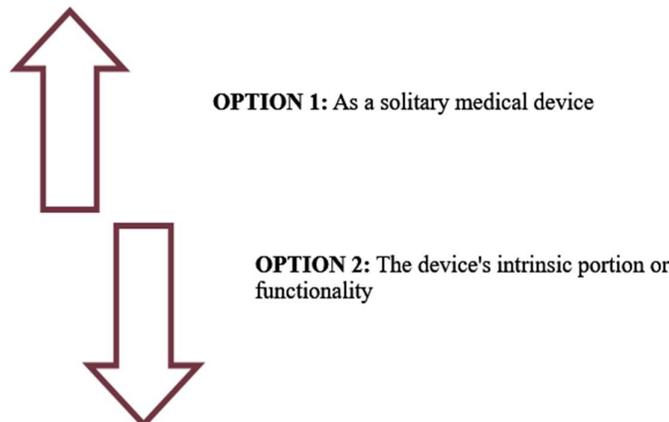

Decision steps for qualification of software as MDSW

The platform's location or the way the software interacts with each other and a

device impacts whether MDSW qualifies as a device or an accessory. For MDSW certification, there are five steps [11] [12] [14].

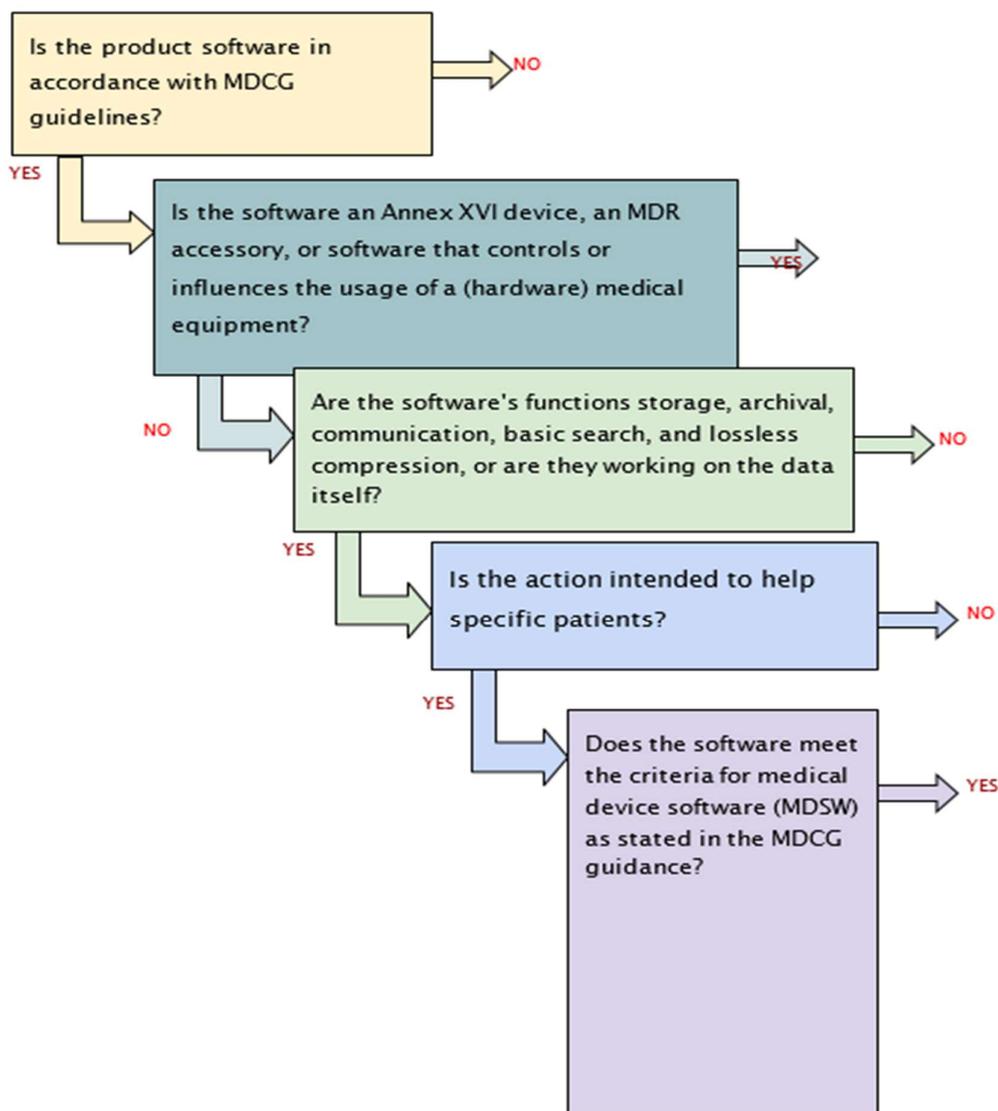

YES - Covered under MDR


NO - Not covered under MDR

What qualifies as a medical device in terms of software?

- The European Union Medical Device Regulation (EU MDR), which was recently passed, provides definitions, guidelines, classifications, and procedural requirements for medical device software standards.
- Various software as medical device categorization guidelines are discussed in EU MDR Annex VIII.
- Specifically, Rule 11 of Annex VIII, which deals with the categorization of software, refers to the classification of software used either alone or in conjunction with medical equipment.

- Class IIa software is intended to give data that is used to make decisions for therapeutic or diagnostic reasons, except in cases where such decisions may result in a person's death or an irreversible decline in health. Such situations fall under Class III unless there has been a significant decline. It falls under Class IIb if it is related to health or a surgical procedure.
- During a standard checkup, for example, Class IIa software may be used to monitor heart rates or other physiological indicators. The classification is advanced to Class IIb, however, if the monitoring is concentrated on critical physiological indications that represent an urgent risk to the patient. It is categorized as Class I for all other software [11] [12].

EU MDR must comply with the requirements those are

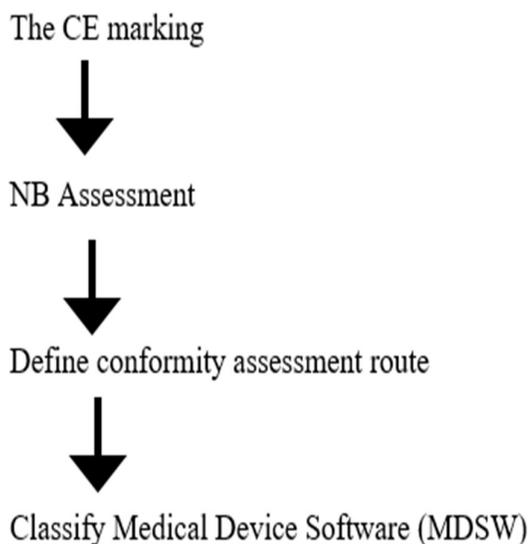

RWE (*real-world evidence*) in EU medical device regulations

A foundational need for post-marketing clinical follow-up in the EU is that data be constantly produced throughout the product's lifecycle. This is by MDR 2017/745. Also required is the production of RWE on safety and efficacy. The data might come from several sources, such as clinical decision support systems, implanted device

datasets, dispensary data, and patient assessments, to highlight a few. RWE can show a product's efficacy and safety for both new and used items and analyze a product's performance after it has been launched to the market (for instance, SaMD or health technology) [14].

(TGA) Regulatory approach for SaMD.

The method taken by Australia to regulate software-based devices is supported by the

IMDRF's policy. The laws substantially align with those of the EU. Unless it is exempt, software products that are medical devices must be registered in the Australian Register of Therapeutic Goods (ARTG) to be distributed legally in Australia.

Australian software and mobile applications that fulfill the requirements of a medical device are governed by the TGA [13] [14].

The TGA regulatory process for medical device supply in Australia may be split into three steps [14]



TGA enacted new rules on February 25, 2021

In December 2019, the Regulations were amended to add a new stipulation for categorizing software-based medical apparatus, known as "Software-based, programmable, and programmed medical devices." It's worth noting that In Vitro Diagnostics (IVDs) are exempt from these rules. On February 25, 2021, these regulations will become effective. Producers and sponsors of medical device products listed in the ARTG before February 25th, 2021 will be offered transitional choices. The regulations address the potential damage that may arise from providing users of these medical devices with erroneous data. [14]

Regulations have been established to include medical apparatus meant for

- Screening or identifying an illness or condition
- Tracking the development or status of an illness, condition, etc.
- Describing or advising a course of therapy or intervention
- Offering treatment (via the provision of information). [14] [17]

In Japan

The oversight of the SaMD regulation procedure is done by the Pharmaceuticals and Medical Devices Agency (PMDA) and the Ministry of Health and Labor Welfare (MOHLW). General medical devices, controlled medical devices, highly controlled (high-risk) medical devices, and specially controlled (life-threatening)

medical devices are the four classifications of SaMD. In December 2019, the Sakigake designating system was put in place due to changes made in the nation's Pharmaceutical and Medical Devices Act which would quicken the regulatory approval process for medical devices. This approach takes into account four components: innovation, efficiency, illness seriousness, and Japan's development plan. The regulations also provide for expedited evaluation of orphan drugs, Sakigake products, and products with a certain usage (such as pediatric usage). The PMDA and MOHLW have collaborated to create the IDATEN framework, which lessens the regulatory pressure and ensures the safety and effectiveness of medical devices through consistent tracking and analysis by producers and the PMDA. This has enabled persistent progress in medical device technology. [14]

In Singapore

A directive on software-based medical devices and the application of AI in the healthcare industry has been made available by the Ministry of Health and the Health Sciences Authority. It identifies medical devices and outlines standards for software certification, data correctness, safety, and effectivity, as well as other SaMD-related aspects. Despite this, neither of these regulatory agencies has exactly categorized SaMD, and neither uses the IMDRF's approach for classifying hazards [14].

Samd/Mdsw risk management connected with its use

Ensuring data accuracy and confidentiality, understanding any racial and cultural dissimilarities in biological features, and exercising caution when dealing with data will all be crucial elements when creating a sound regulatory framework. The General Data Protection Regulation 2016/679 (GDPR) provides standards and restrictions for devices in numerous countries [14].

Initiative to update from a product to a system approach

Instead of relying on medications, it is widely accepted that factors such as tools, personnel, abilities, instruction, culture, workflow, and procedures have a big influence on how software and IT are utilized (for instance, in terms of data quality management). Authorities might additionally impose further restrictions, like ongoing system observation, frequent retraining, software and utilization reviews, and a general evaluation of usage details (like to discover possible movements in treatment frequencies and decision forms of users).


Authorities need data and model confirmation and robustness analysis due to concerns about data quality or antagonistic attacks. Authorities might also require that versions with varying levels of liberty be tested: when a tool offers probabilistic

suggestions, for example, users' discretion may be more or less restricted.

Supervisory authorities may also necessitate medical assessments for SaMD when it is used for its authentic, planned medical purposes, monitor any alterations in

behavior over an extended period, and have digital medical records that register all choices that could be associated with the utilization of SaMD.

Recall these important details

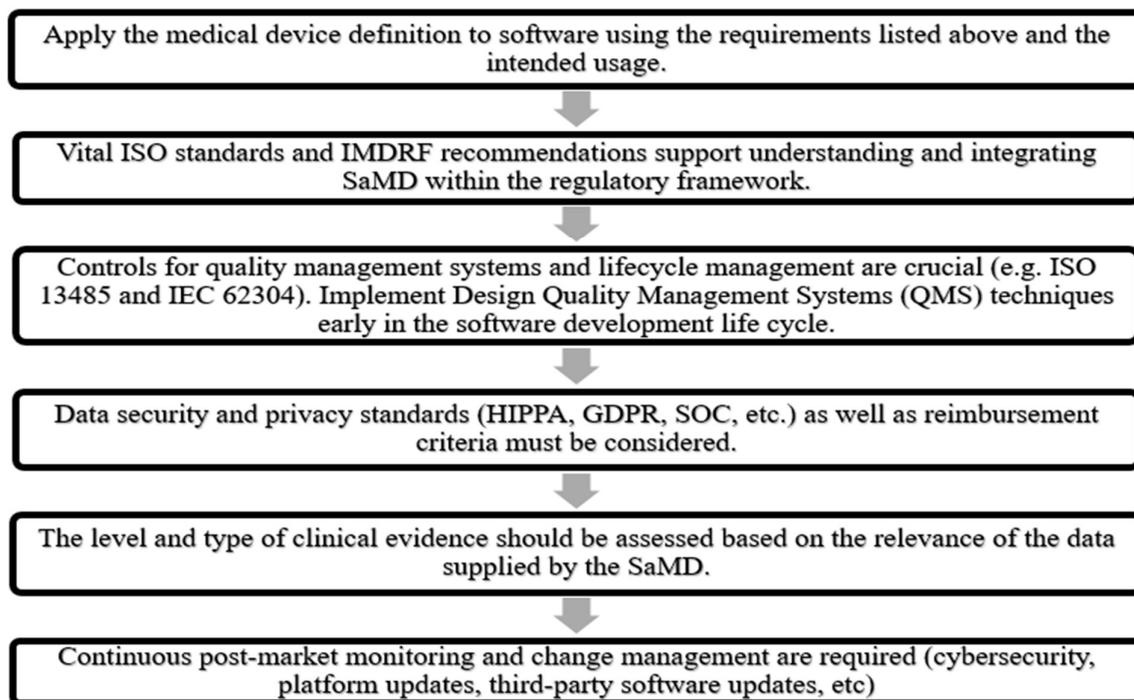

CONCLUSION

The COVID-19 epidemic has taught us the need to be always flexible. Software-enabled medical devices enable people to take care of themselves and make healthcare products even more comfortable. Even though it's not required by law, SaMD makers that follow these rules will find it simpler to have their medical devices approved by regulators. It is also vital to adopt an intersectional strategy that brings together several government departments to

inform the regulatory recommendations this framework should have laws that defend privacy, diversity, data integrity, and human rights. According to research, a piece of medical equipment must be marketed for about three to seven years. Unfamiliar developers may grow dissatisfied and abandon working on SaMD products due to problems in having their products authorized and supplied on time. Products that offer a moderate-to-high danger to the health of patients may necessitate a more

extensive review procedure. Last but not least, SaMD devices may continually gather medical data such as body temperature, heart rate, test results, and other variables. As a result, these items and patient data must be securely protected against any cybersecurity threats. As a result, proper training is required to assure SaMD utilization, improve productivity, and report RWD.

Acknowledgment

I am thankful to my guide who initiated me to work on this topic and I am also thankful to my co-author who contributed to my manuscript preparation throughout.

Conflict of Interest

The authors declare no conflict of interest.

Financial Support

Nil.

REFERENCES

- [1] SaMD N10: Software as a Medical Device (SaMD): Key Definitions - <http://www.imdrf.org/docs/imdrf/final/technical/imdrf-tech-131209-SaMD-key-definitions-140901.pdf>.
- [2] Software as a Medical Device (SaMD): What It Is & Why It Matters Bernhard Kappe Published on: May 1st, 2021-- <https://orthogonal.io/insights/SaMD/software-as-a-medical-device-SaMD-basics/>.

- [3] SaMD N12: Software as a Medical Device (SaMD): Possible Framework for Risk Categorization <http://www.imdrf.org/docs/imdrf/final/technical/imdrf-tech-140918-SaMD-framework-risk-categorization-141013.pdf>.
- [4] SaMD N23: Software as a Medical Device (SaMD): Application of Quality Management System - <http://www.imdrf.org/docs/imdrf/final/technical/imdrf-tech-151002-SaMD-qms.pdf>.
- [5] IEC (2010). Application of risk management for IT-networks incorporating medical devices -- Part 1: Roles, responsibilities, and activities (IEC80001-1) Geneva, Switzerland: ISO.
- [6] ISO 62304/A1: 2015: Medical device software – Software life-cycle processes -- <https://www.iso.org/standard/64686.html>.
- [7] IEC 62304:2006 Medical device software — Software life cycle processes-- <https://www.iso.org/standard/38421.html>.
- [8] The United States Food and Drug Administration is a federal agency of the Department of Health and Human Services-- Digital Health Center of Excellence – FDA--

- <https://www.fda.gov/medical-devices/digital-health-center-excellence>.
- [9] The United States Food and Drug Administration -- Center For Devices & Radiological Health-- Artificial Intelligence/Machine Learning (AI/ML)-Based Software as a Medical Device (SaMD) Action Plan, January 2021.
- [10] Software as a Medical Device (SAMD): Clinical Evaluation Guidance for Industry and Food and Drug Administration Staff Document issued on December 8, 2017.
- [11] Software as a Medical Device (SaMD): Useful or Useless Term? Rebecca Hermon, Patricia A H Williams, Vincent B McCauley, Proceedings of the 54th Hawaii International Conference on System Sciences | 2021, Pg 3722-3728.
- [12] Owono, G.F., Korrapati, R., Bush, R. & Stottlemeyer, D. (2015). Impact of EU Medical Device Directive on Medical Device Software, ProQuest Dissertations and Theses.
- [13] The Regulation of Medical Devices in Australia. Therapeutic Goods Administration, Department of Health-Therapeutic Goods Administration, Australia; 2002.
- [14] Regulatory Framework of Software as Medical Device <https://www.makrocare.com/Whitepaper/regulatory-framework-software-med-device.pdf>.
- [15] IMDRF Good Regulatory Review Practices Group. Essential principles of safety and performance of medical devices and IVD medical devices. 2018. Available from: <http://www.imdrf.org/docs/imdrf/inal/technical/imdrf-tech-181031-grp-essential-principles-n47.pdf>. Accessed January 31, 2023.
- [16] The Essential Principles for medical devices. Australian medical devices guidance document, 22. 2003. Available from: <https://www.omnex.com/training/isol3485/australia/Australia-Device-Essential-Principles.pdf>. Accessed December 31, 2022.
- [17] Lee, I., Pappas, G. J., Cleaveland, R., Hatcliff, J., Krogh, B.H., Lee, P., & Sha, L. (2006). High-confidence medical device software and systems. *Computer*, 39(4), 33-38. doi: 10.1109/MC.2006.12
- [18] Simons, D. (1997). Medical device software regulation: an industry

perspective. Food and drug law journal, 52(2), 189.

- [19] Cobbaert, K. (2011). When does software become a medical device? European Medical Device Technology, 2(9), 21.